





DESS

> DENTAL SMART SOLUTIONS

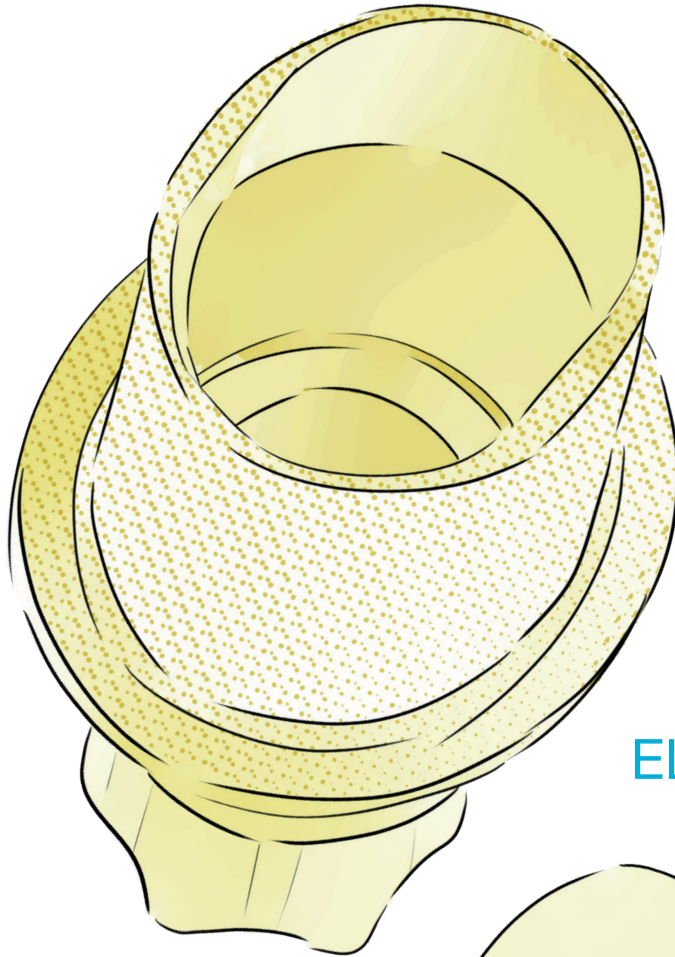

ELLIPTIBase® 2022/1

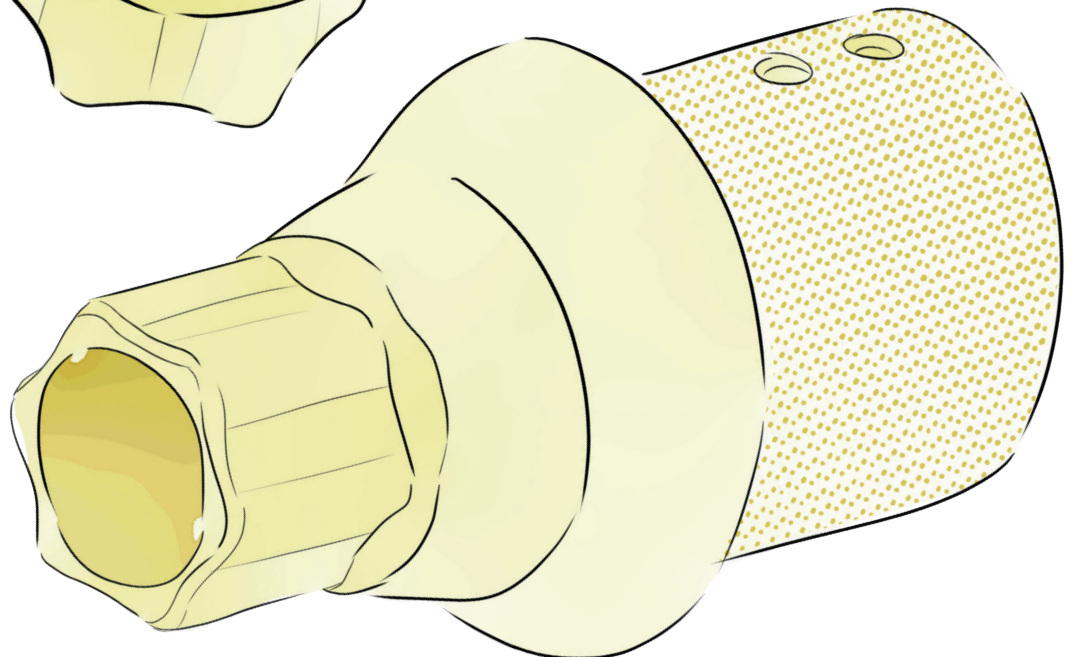




Tight spaces not a problem


Restorations in positions where the interdental space is limited, have always been challenging, up until now, existing solutions would mean making sacrifices. Either because of the lack of space for the correct amount of restorative material or when it comes to achieving the best aesthetic result.

ELLIPTIBase® has been specially designed to solve these problems.

The elliptical design allowed us to increase the space for restorative material, whilst maintaining almost the same cementation area.

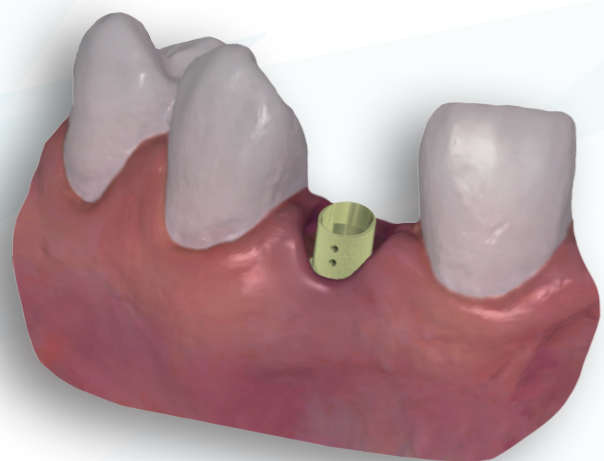


Comparison between a standard size DESS® TI-Base and the ELLIPTIBase®.

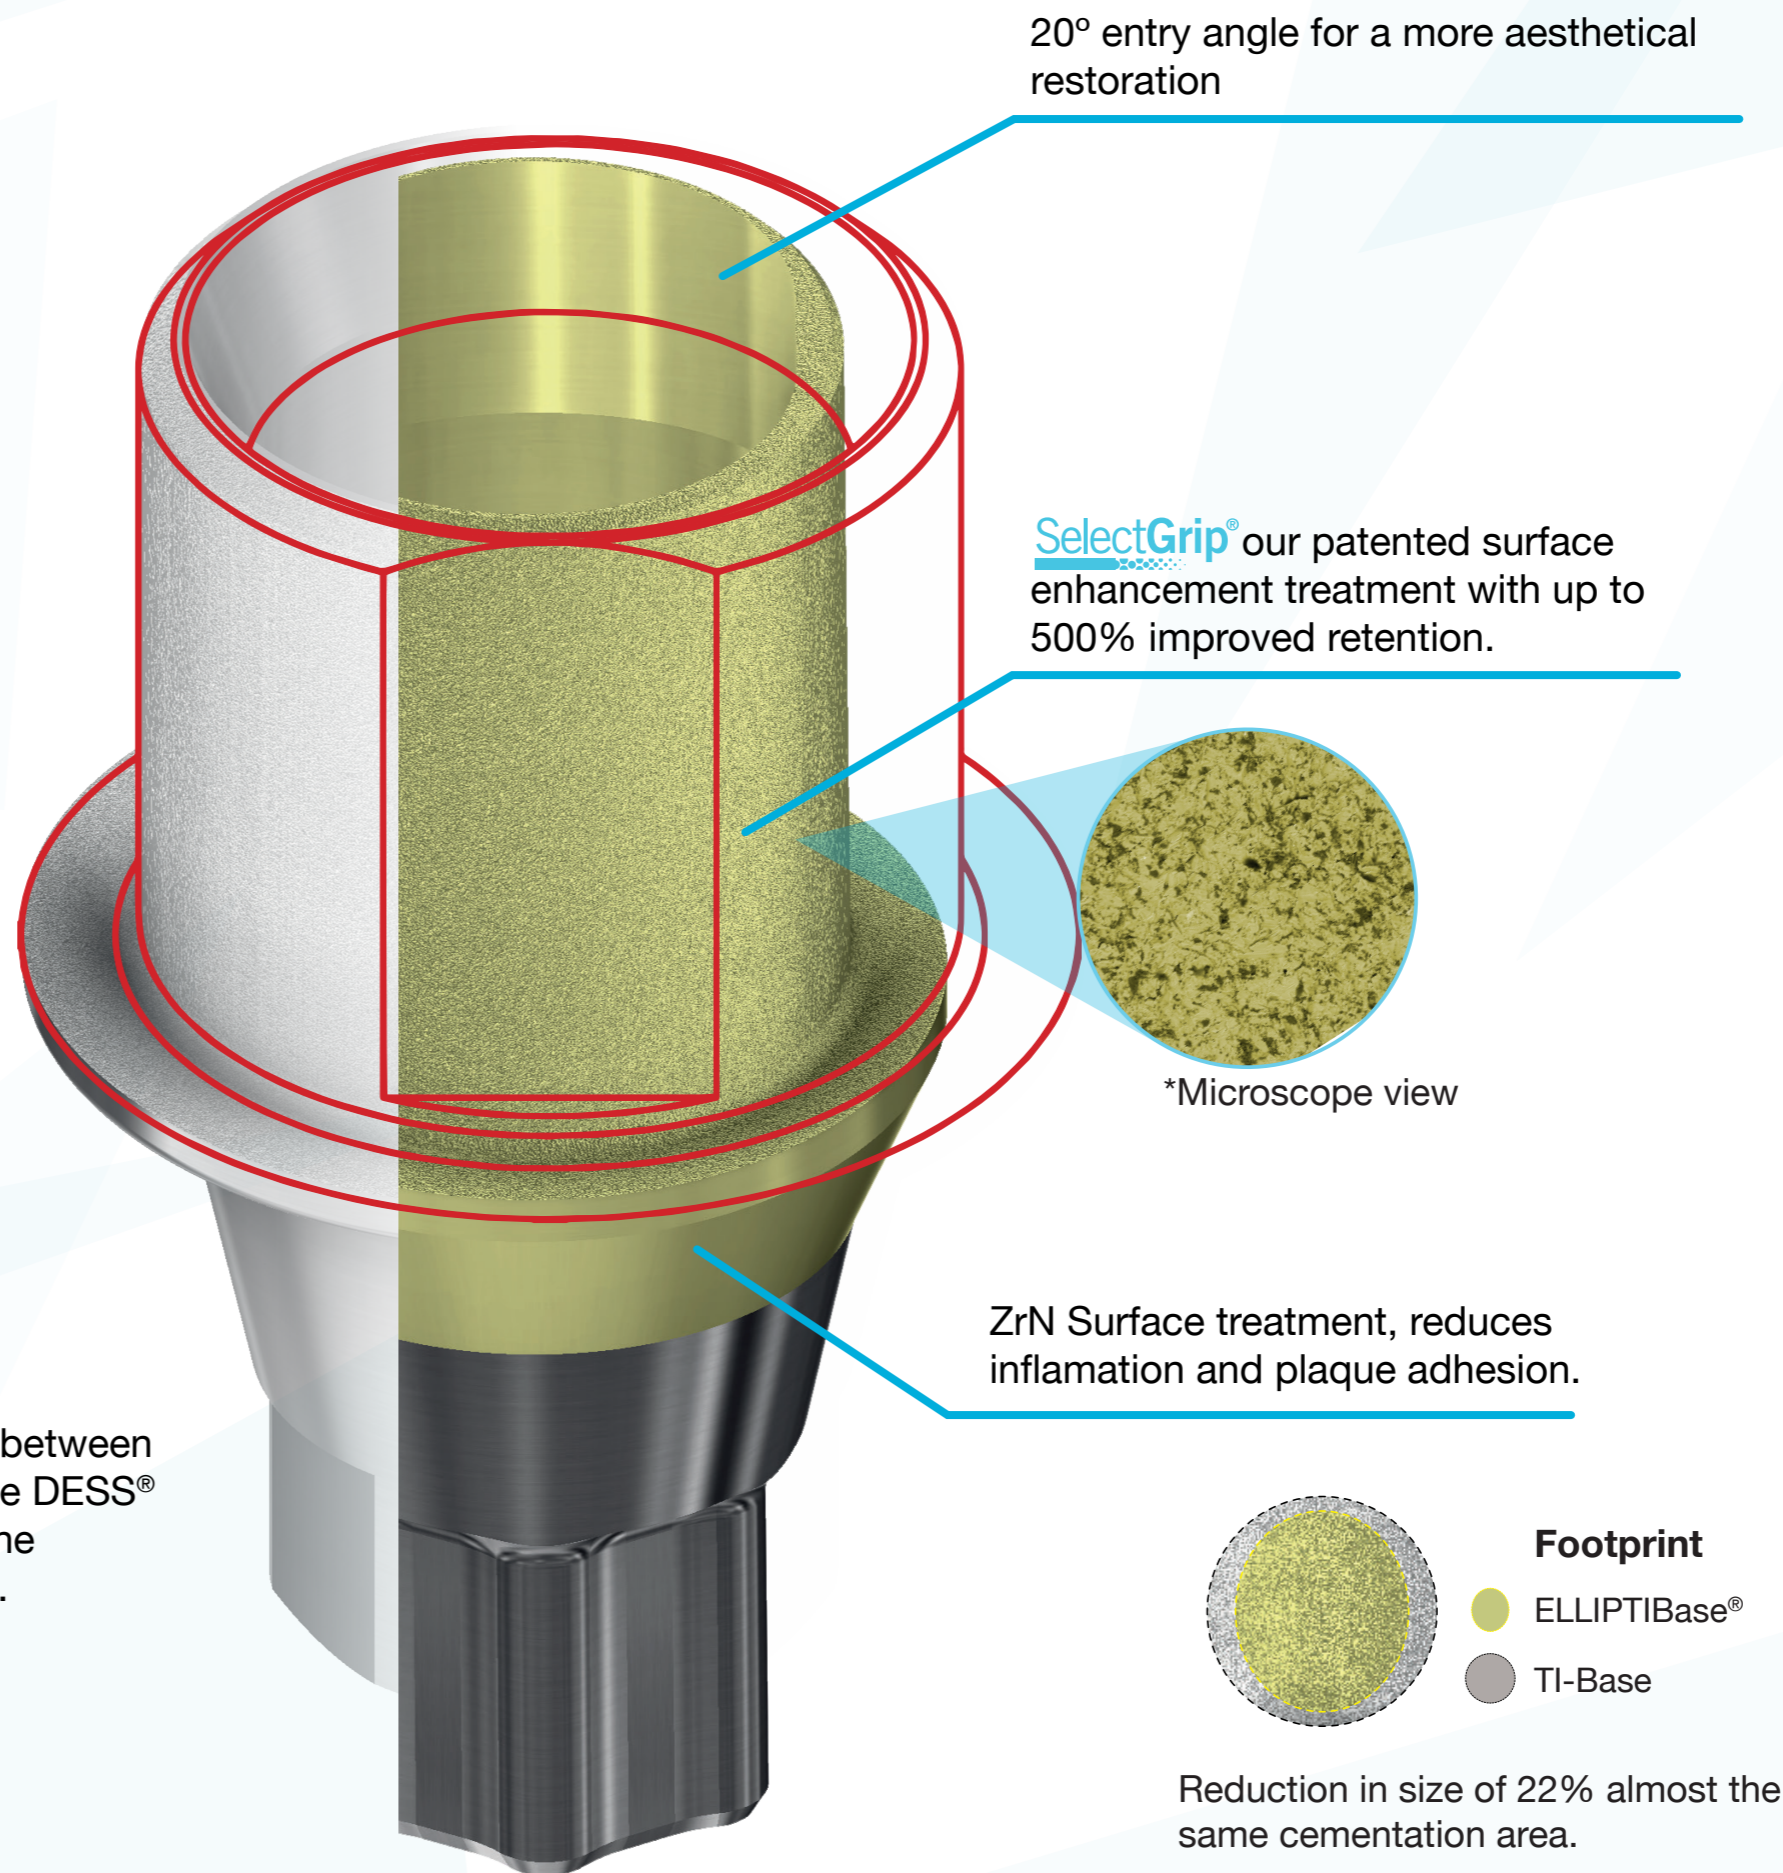

Aesthetic Advantages

The DESS® ELLIPTIBase® addresses all those problems that arise when working on restorations where a 3.0 or 3.5 implant is used, particularly the incisors positions. These restorations require for an improved aesthetical result and a strong restoration.


The 20° angulation on the access channel, combined with a lower shaft height will allow you to achieve the best aesthetical results without compromise.

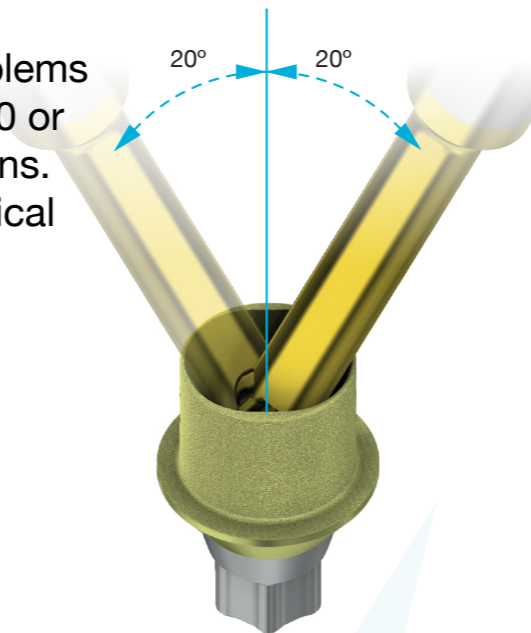

Corner vs. Flat

Due to the shape of the ELLIPTIBase® we created corner and flat versions that depending on the orientation in which the implant has been placed, can be used to achieve the best result.

On any given hex connection the angle is of 45°, the corner connection would aid reducing the final angle of the shaft.™

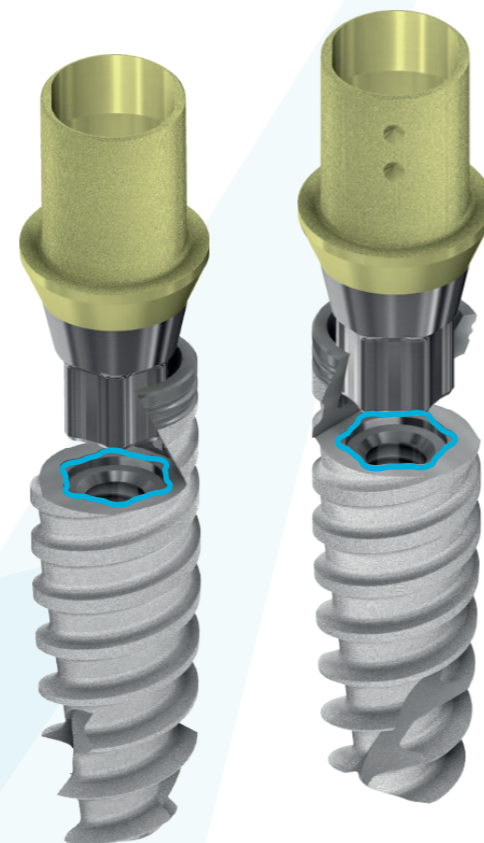

Corner



Flat


| Shaft orientation

⬡ Implant position

Surface Technology

The zirconium nitride surface treatment improves the overall mechanical resistance of the ELLIPTIBase® whilst reducing inflammation and plaque adhesion, offering better biocompatibility with the gums.


- Reduces plaque adhesion
- Decreases inflammation

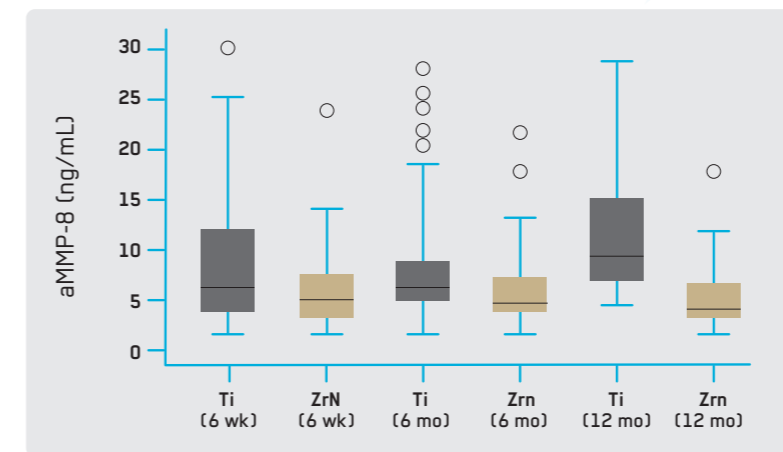


aMMP-8* values of fluid from peri-implant sulcus in titanium (Ti) and Zirconium Nitride (ZrN) coated attachments at different times after prosthetic restoration.


(Matrix Metalloproteinase-8 Levels in Peri-implant Sulcus Fluid Adjacent to Titanium and Zirconium Nitride Surface, Richard Meissen, MSc1 Mariana Mintcheva, MSc1 Lutz etuschil, PhD Dr2, Int J Periodontics Restorative Dent 2014; 34:91-95. doi: 10.11607/prd.1504)

* Presence of MMP-8 indicates an ongoing inflammation

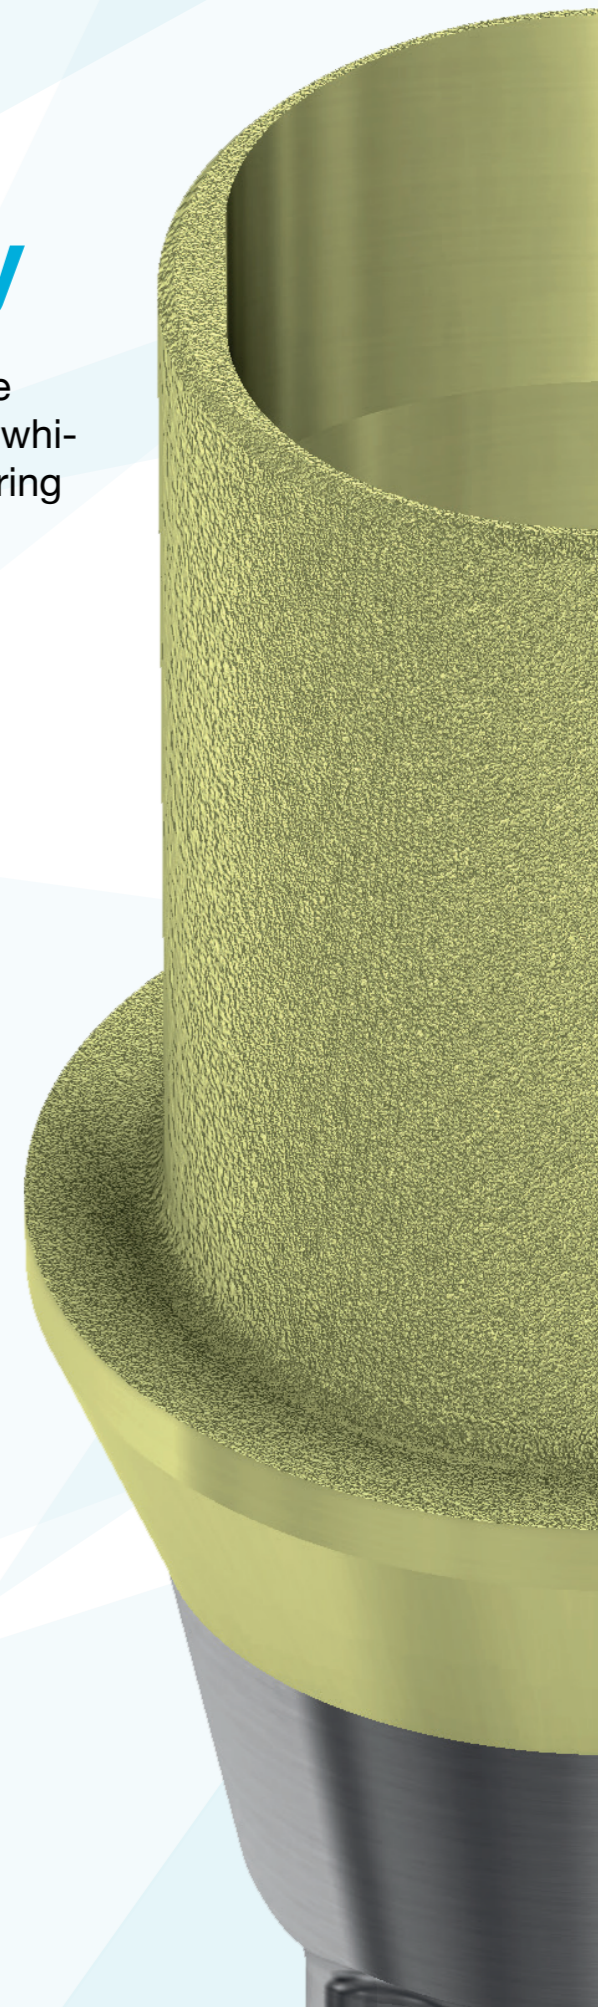





		3.0	NP	RP	WP
NobelActive® NobelReplace® CC Active Hex		3.0	3.5	4.3/5.0	5.5
A corner		56.068			
B flat		57.068			
	Torx® Screw ELLIPTIBase®	19.468			




		NNC	RN	WN
Straumann® Soft Tissue level & synOCTA® Octagon		3.5	4.1/4.8	4.8/6.5
A corner		56.070		
B flat		57.070		
	Torx® Screw ELLIPTIBase®	19.441		




		NP	RP	NP/RP
Straumann® Bone level® Conical BL		NC/3.3	RC/4.1-4.8	NC/RC
A corner		56.043		
B flat		57.043		
	Torx® Screw ELLIPTIBase®	19.443		



		NP	RP	WP
Zimmer® Screw-vent Internal Hex USA		3.5	4.5	5.7
A corner		56.017		
B flat		57.017		
	Torx® Screw ELLIPTIBase®	19.417		



		EV/3.0	EV/3.6	EV/4.2	EV/4.8	EV/5.4
Astra Tech implant system™ EV Conic EVO		3.0	3.6	4.2	4.8	5.4
A corner		56.406				
B flat		57.406				
	Torx® Screw ELLIPTIBase®	19.331				



		3.0	NP	RP	WP
Biohorizons® internal Internal hex BH		3.0	3.5	4.5	5.7
A corner		56.099			
B flat		57.099			
	Torx® Screw ELLIPTIBase®	19.400			

All DESS products are manufactured according to ISO 9001:2015 and ISO 13485:2016 with CE marking for all products Class IIb

All DESS® AURUMBase® screws and screwdrivers are based on the standard ISO 10664

3i® and 3i Certain®, Miniplant®, MicroMiniplant™ and Osseotite® are registered trademarks of 3i Implant Innovations, USA
ASTRA TECH™, OsseoSpeed™, ANKYLOS® C/X, XiVE®, FRIADENT®, ASTRATECH implant system™ EV and UniAbutment®

are registered trademarks of DENTSPLY SIRONA Implants

BioHorizons® is a registered trademark of BioHorizons, INC.

Brånemark System®, NobelReplace® and Replace Select™, NobelActive™, NobelReplace® CC, NobelSpeedy™ and Multi-unit® are registered trademarks of Nobel Biocare AB, Sweden

ITI®, Straumann® and synOcta® are registered trademarks of Straumann Holding AG, Switzerland

MIS® is a registered trademark of MIS Implant Technologies Ltd.

Zimmer Screw-Vent® and SwissPlus® are registered trademarks of Zimmer Dental INC, USA

Locator® is a registered trademark of ZEST IP Holdings

Camlog® and Conelog® are registered trademarks of CAMLOG Biotechnologies AG.

DESS products can be used only by licensed dentists, physicians and labs.

Please refer ever to the instructions of use available on the website

www.dessdental.com

or supplied with the product.

Some products may not be available in your country. Some of the products are cleared for US and Canada.

Please contact your local distributor for more details.



